



## NanoTack® and NanoTack® Flex Anatomic Labrum Restoration System




NanoTack Suture Anchor Undeployed




NanoTack Suture Anchor  
[cross section] Undeployed

	Diameter (mm)
1	1.4
2	1.5
3	1.5
4	2.0 max.




NanoTack Suture Anchor after  
actuation and expansion




NanoTack Suture Anchor after actuation and expansion  
[cross section]

# NanoTack and NanoTack Flex Anatomic Labrum Restoration System

Pull Out Strength\* (Pounds)

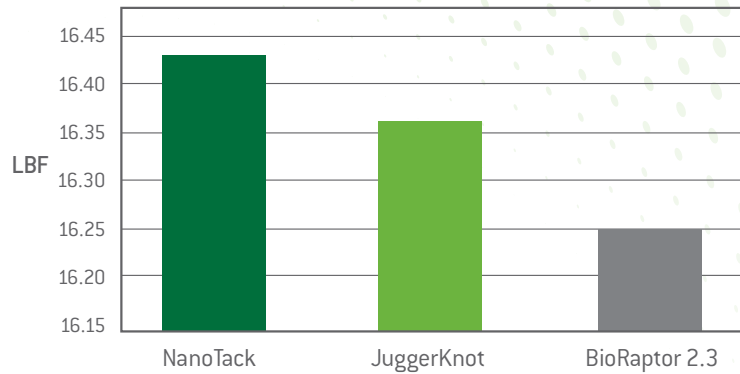

Pull Out Strength\* (Newtons)



## NanoTack and NanoTack Flex Ordering Information

Description	Catalog No.
NanoTack Suture Anchor, 1.4mm w/Inserter	CAT01386
NanoTack Drill Bit	CAT01373
NanoTack Guide	CAT01371
NanoTack Obturator	CAT01372
NanoTack Suture Anchor, 1.4mm w/Flex Inserter	CAT01858
NanoTack Flex Drill Bit	CAT01859
NanoTack Flex Guide	CAT01860
NanoTack Flex Obturator	CAT01861
NanoPass® Suture Manager, Reach Crescent	CAT02298
NanoPass Suture Manager, Reach 45° Left	CAT01355
NanoPass Suture Manager, Reach 45° Right	CAT01356
Knot Pusher	CAT01518

\*Data from non-clinical [bench] comparison testing in foam bone model [pr01569-A Section 4.1.1 [JuggerKnot], pr01618-A Section 4.6.1.1 [BioRaptor]]

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: NanoTack, Stryker. All other trademarks are trademarks of their respective owners or holders.

### Pivot Medical, Inc.

A Stryker Sports Medicine Company  
247 Humboldt Court  
Sunnyvale, CA 94089 USA